


LumiFlow™

V series Quick Guide



1. Flow Image acquisition

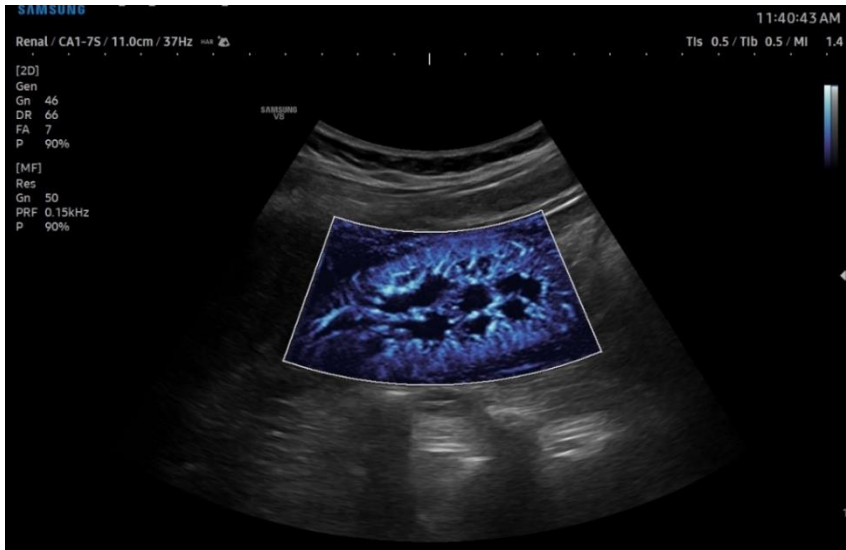

① Flow image Acquisition

Acquire an image with the structure you wish to apply LumiFlow.


**LumiFlow can be applied to both live mode or frozen images.

★Tips

※ LumiFlow™ is supported in all of the probes and presets.

Probe	Application
All Probes	All Presets <ul style="list-style-type: none"> Operates in Flow Mode (Color Doppler, Power Doppler, S-Flow™ and MV-Flow™)


2. Apply LumiFlow™

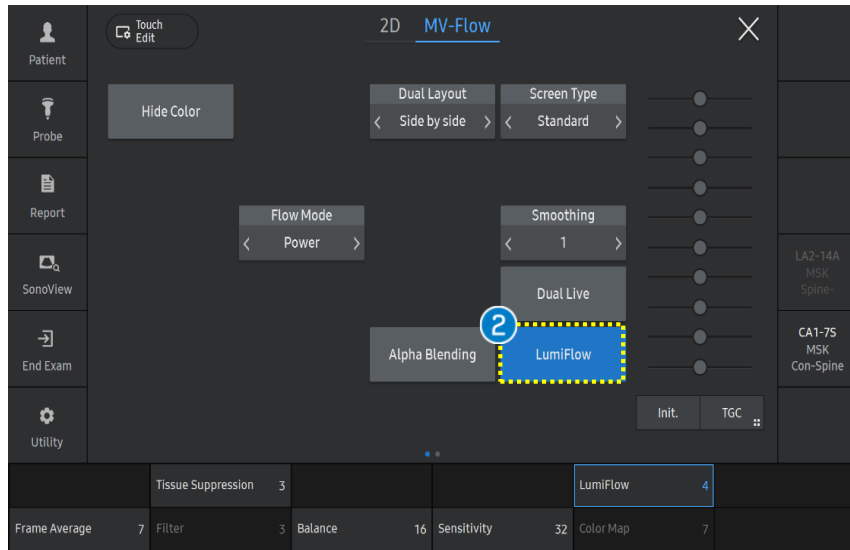


LumiFlow provides a 3D-like appearance to all flow imaging modes. By applying LumiFlow, it can help you to easily observe the hemodynamic flow within the vascular structure.

1 LumiFlow™

Tap [LumiFlow] button on the touch screen to apply LumiFlow on the flow image in frozen or live mode.

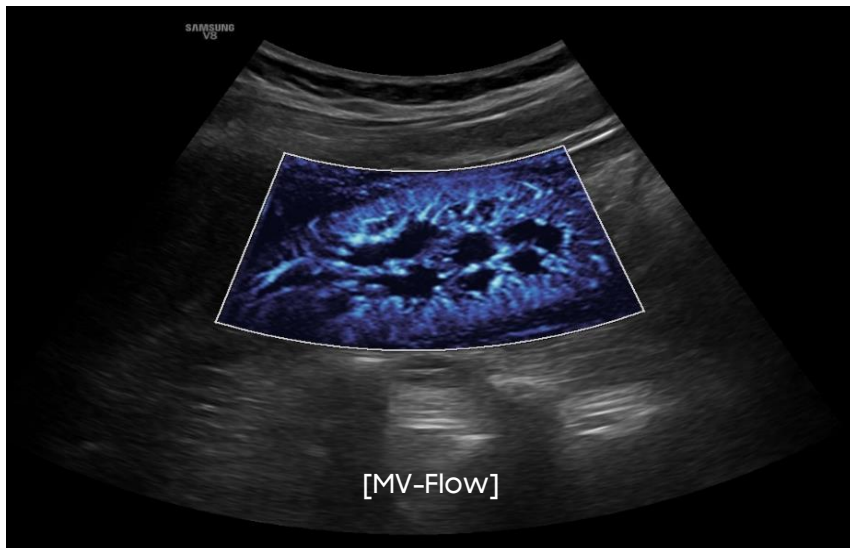

3. Adjust the Index of LumiFlow™

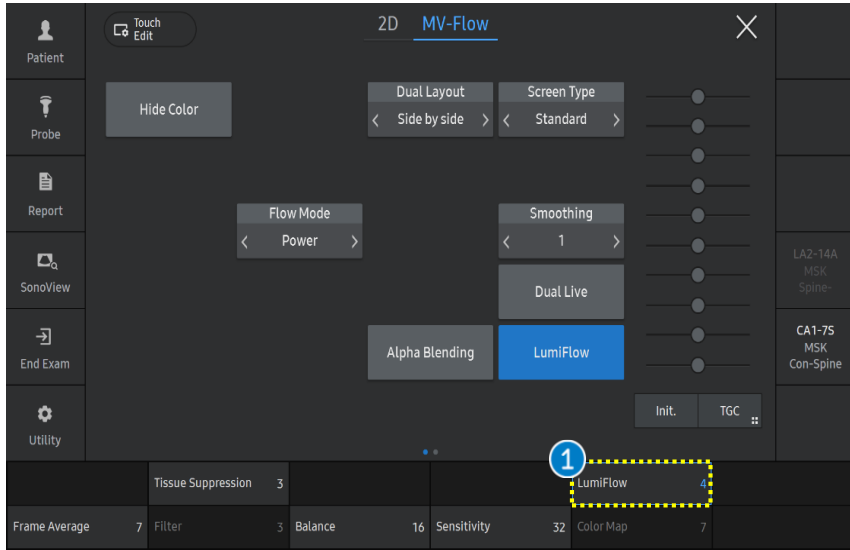

1 Adjust Index (1-5)

You can adjust the index value depending on the vessel size and characteristics.

Low Index (1-2)	The lower index value is more appropriate for imaging the tiny vessels .
High Index (3-5)	The higher index value is more appropriate for imaging the relatively large vessels and heart chambers.



- The features, options may not be commercially available in some countries.
- Sales and shipments are effective only after the approval by the regulatory affairs. Please contact your local sales representative for further details.
- This Quick guide does not include all of the details of instruction, for more detail, please refer to V series User Manual.
- Do not distribute this document to customers unless relevant regulatory and legal affairs officers approve such distribution.
- This User Quick Guide is based on V series V1.05.
- Disclaimer: Some Images in this content were obtained from other system.

SAMSUNG MEDISON CO., LTD.

© 2024 Samsung Medison All Rights Reserved.

Samsung Medison reserves the right to modify the design, packaging, specifications, and features shown herein, without prior notice or obligation.