


CrystalVue™

HERA Z20 Quick Guide




1. Probe and Preset

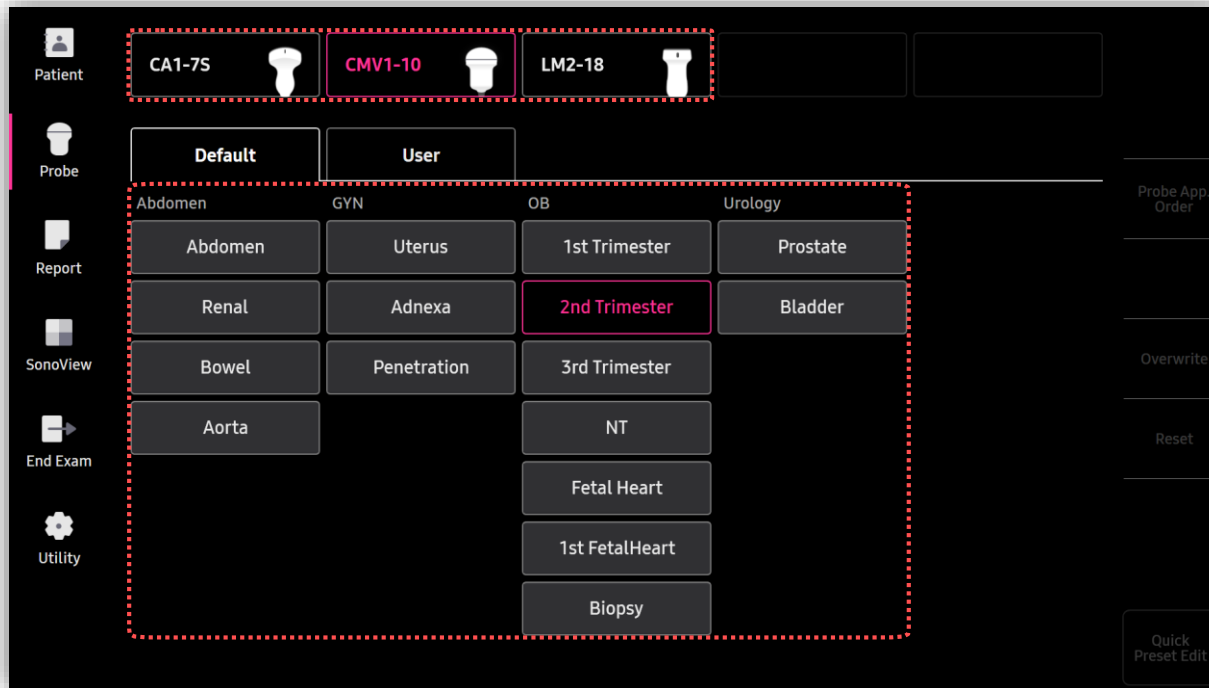

※ CrystalVue can be operated under the following conditions :

Probe	Application
CV1-8A EV2-12 CMV1-10	All presets


2. Volume acquisition

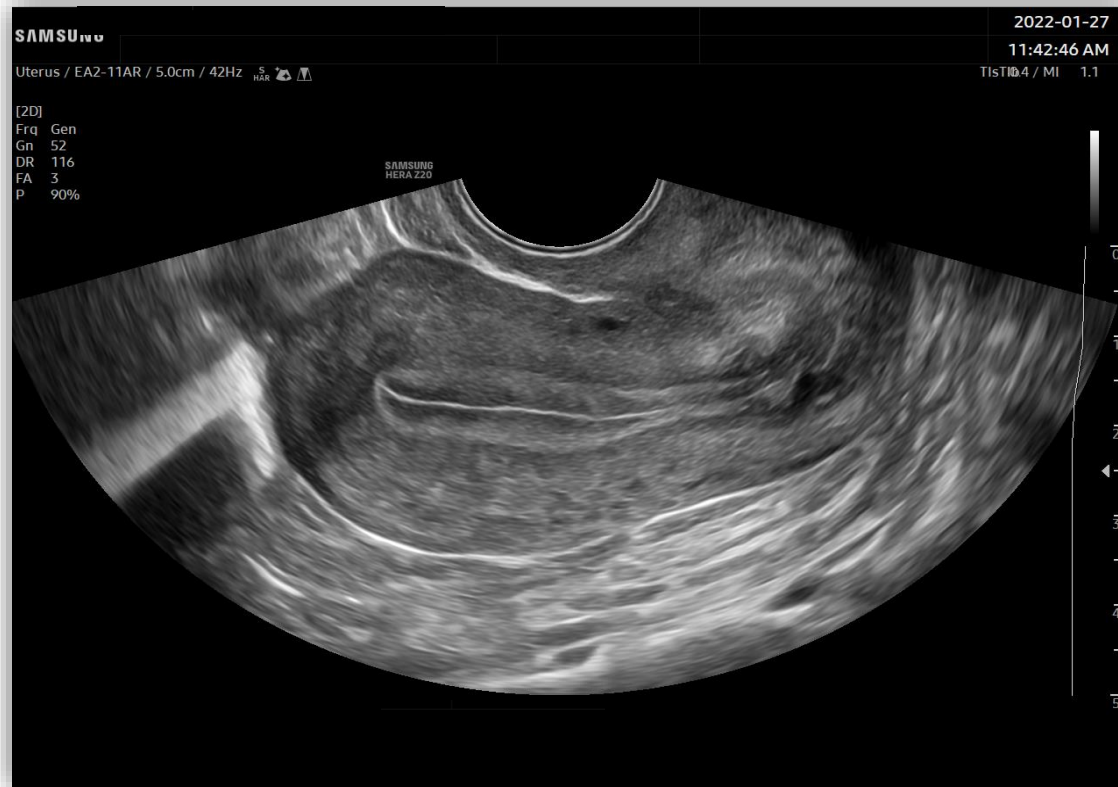


1 Volume acquisition

Acquire the volume data with the structure you desire to apply CrystalVue.

3. Apply CrystalVue™

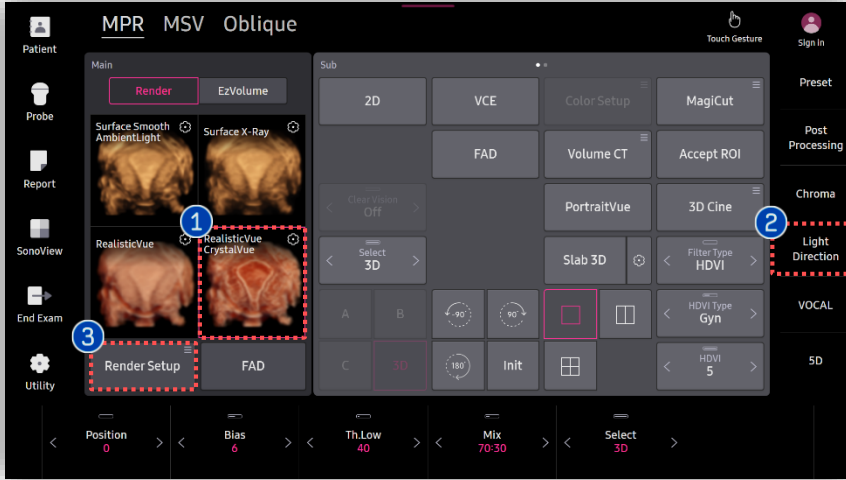


<p>1 CrystalVue</p>	<p>Tap [RealisticVue CrystalVue] on the touch screen.</p>
<p>2 Light Direction</p>	<p>Tap [Light Direction] within short cut keys when you adjust the direction of light freely by trackball.</p>
<p>3 Render Setup</p>	<p>Tap [Render Setup] on the touch screen to adjust parameters of CrystalVue.</p>
<p>4 Pre-defined Light direction</p>	<p>Tap pre-defined light direction among 9 designated options.</p>

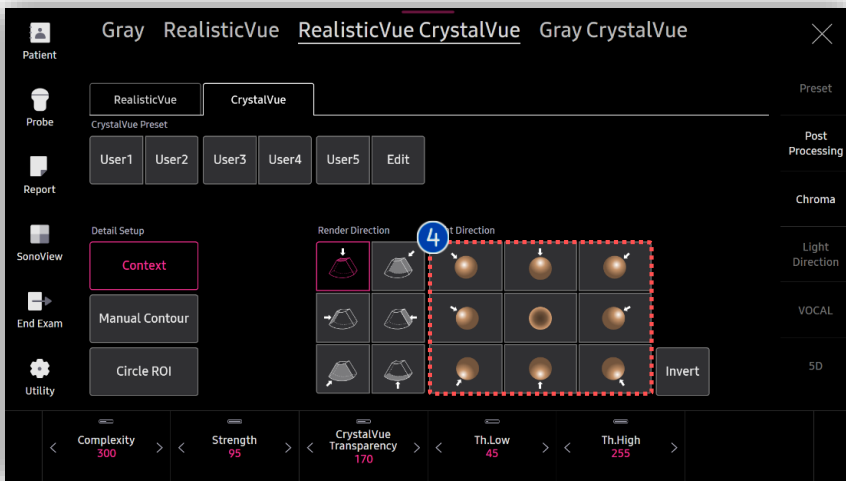


CrystalVue™

4. Adjust CrystalVue™ Parameters

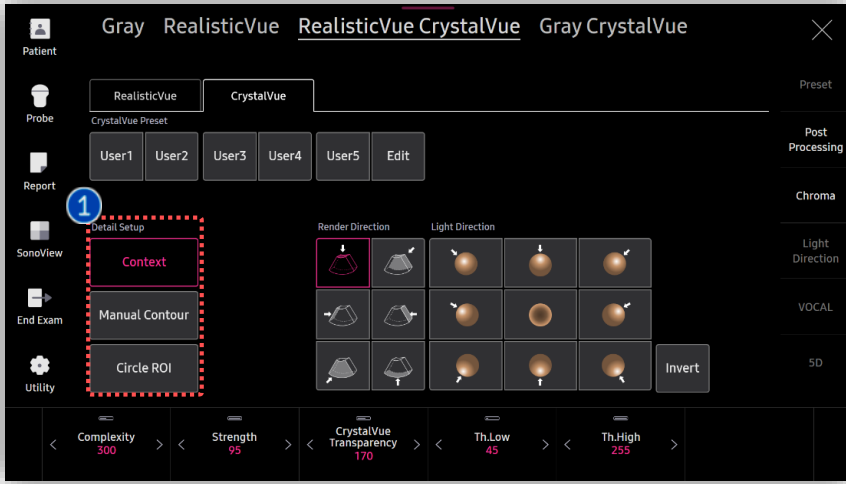


1 ROI Type
 Select type of ROI between Context, Manual Contour and Circle ROI.

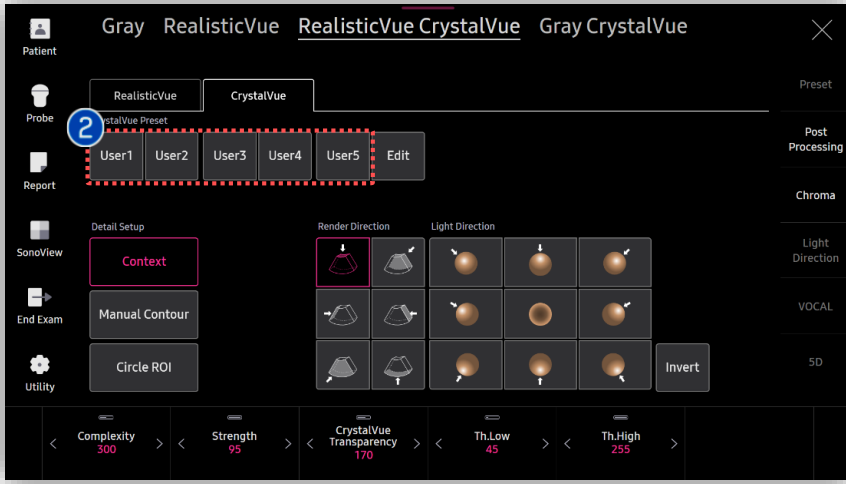

2 CrystalVue Preset
 Select one among various pre-defined presets for quick feedback.
 • The higher the preset number, the more internal information.




5. Edit CrystalVue™ Preset

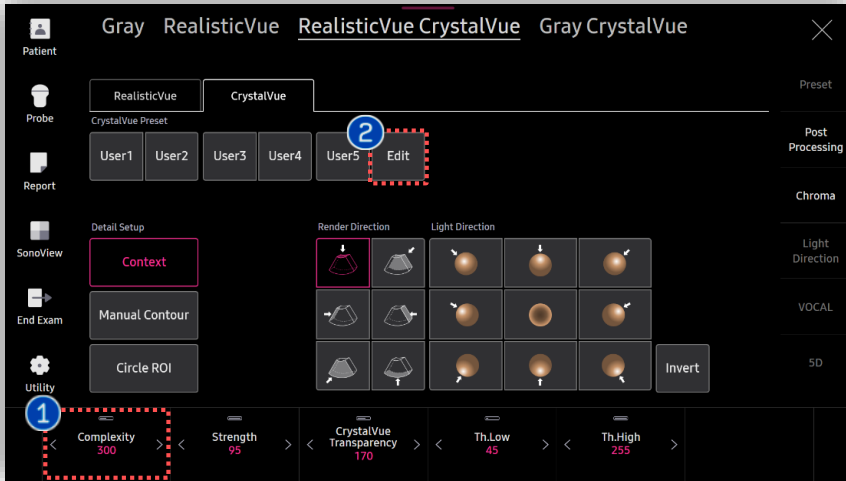

1 CrystalVue Parameters

For fine adjustment, use these three parameters.

- **Complexity:** The higher Complexity value, the more context information. The lower value, the more surface information.
- **Strength:** As the Strength value is higher, the context information becomes clearly visible.
- **CrystalVue Transparency:** Level of transparency or opacity.

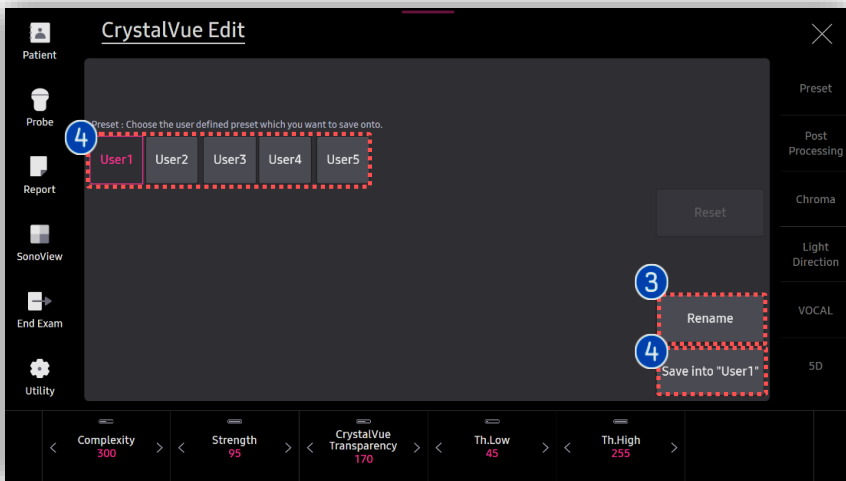

2 Edit

After parameter adjustment, tap [Edit] to save it.

3 Rename

Tap to designate name of the preset.

4 Save into

Tap to save into selected preset.


CrystalVue Flow™

HERA Z20 Quick Guide




CrystalVue Flow™

1. Apply CrystalVue Flow™

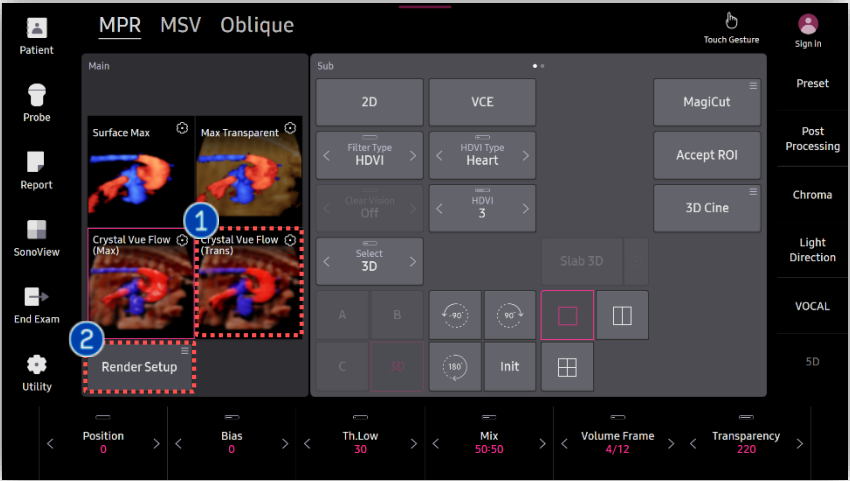

Acquire Volume image with Doppler method such as Color, Power and S-Flow.

- 1 **CrystalVue Flow** After acquisition, tap [Crystalvue Flow].
- 2 **Render Setup** Tap [Render Setup] to adjust parameters of CrystalVue Flow.

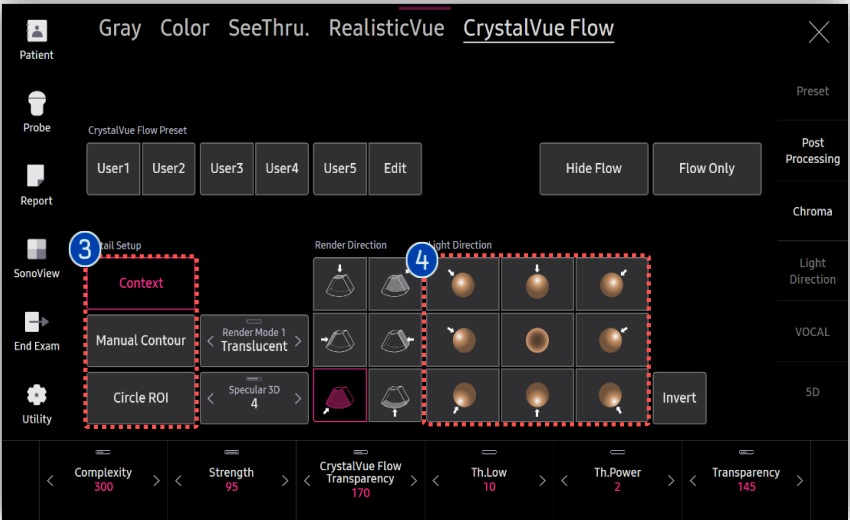


Select type of ROI between Context, Manual Contour and Circle ROI.

- 3 **ROI Type**
- 4 **Pre-defined Light direction** Tap pre-defined light direction among 9 designated options.

CrystalVue Flow™


2. Apply CrystalVue Flow™

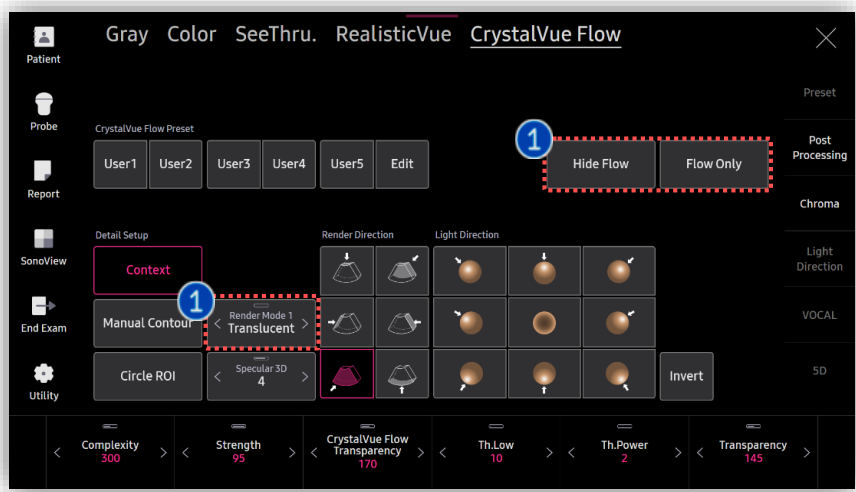

1 Display Mode


You can select display mode among various options below.

- **Translucent:** Color signal will be represented within tissue signal.
- **Max:** Color signal will be represented in maximum intensity.
- **Hide Flow:** Only tissue signal will be represented.
- **Flow Only:** Only Doppler signal will be represented.

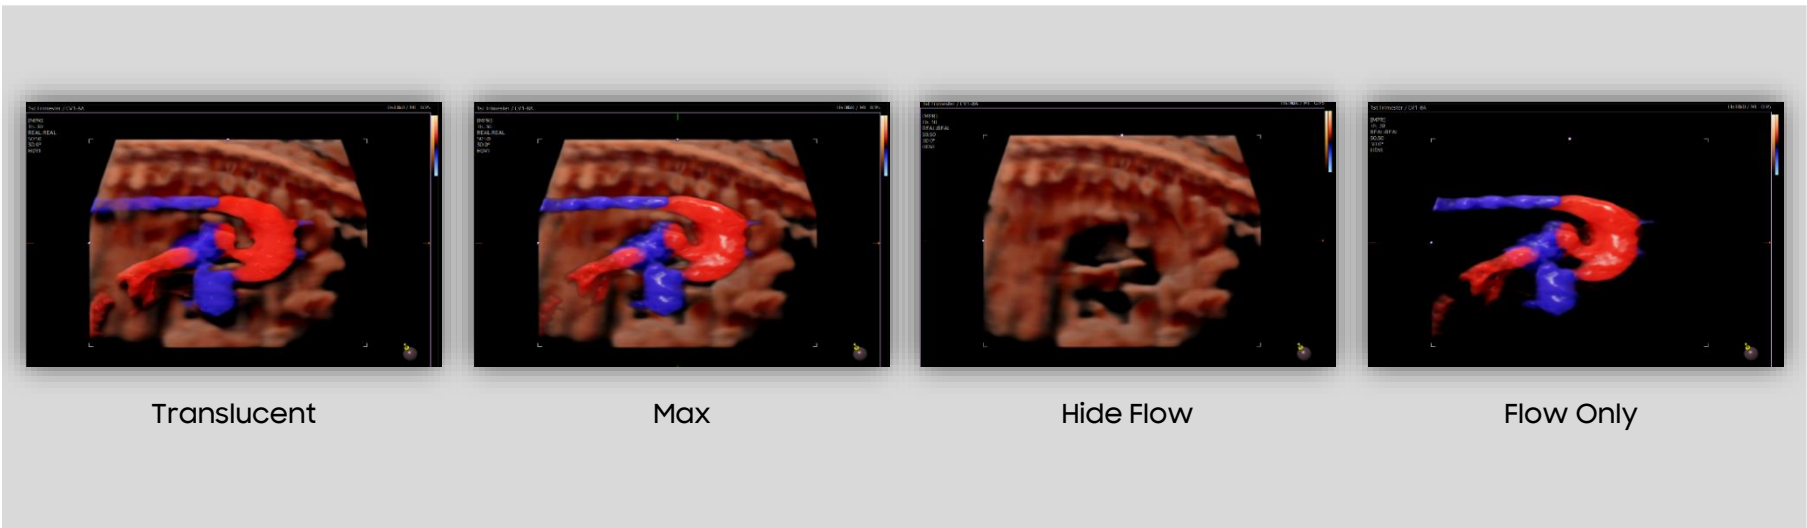

CrystalVue Flow™


3. Adjust Color Parameters

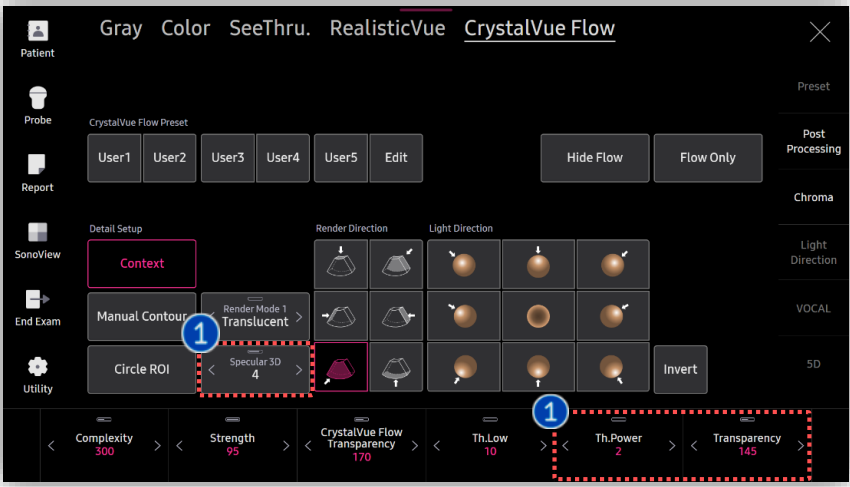


1 Color Parameters

You can adjust parameters of Color signal.

- **Th.Power:** As Th.Power increases, overall color signal will be gradually eliminated.
- **Specular 3D:** As the index increases, there are more watery effect applied.
- **Transparency:** The lowest value(20) is for transparent color signal, and the highest value(250) is for opaque color signal.

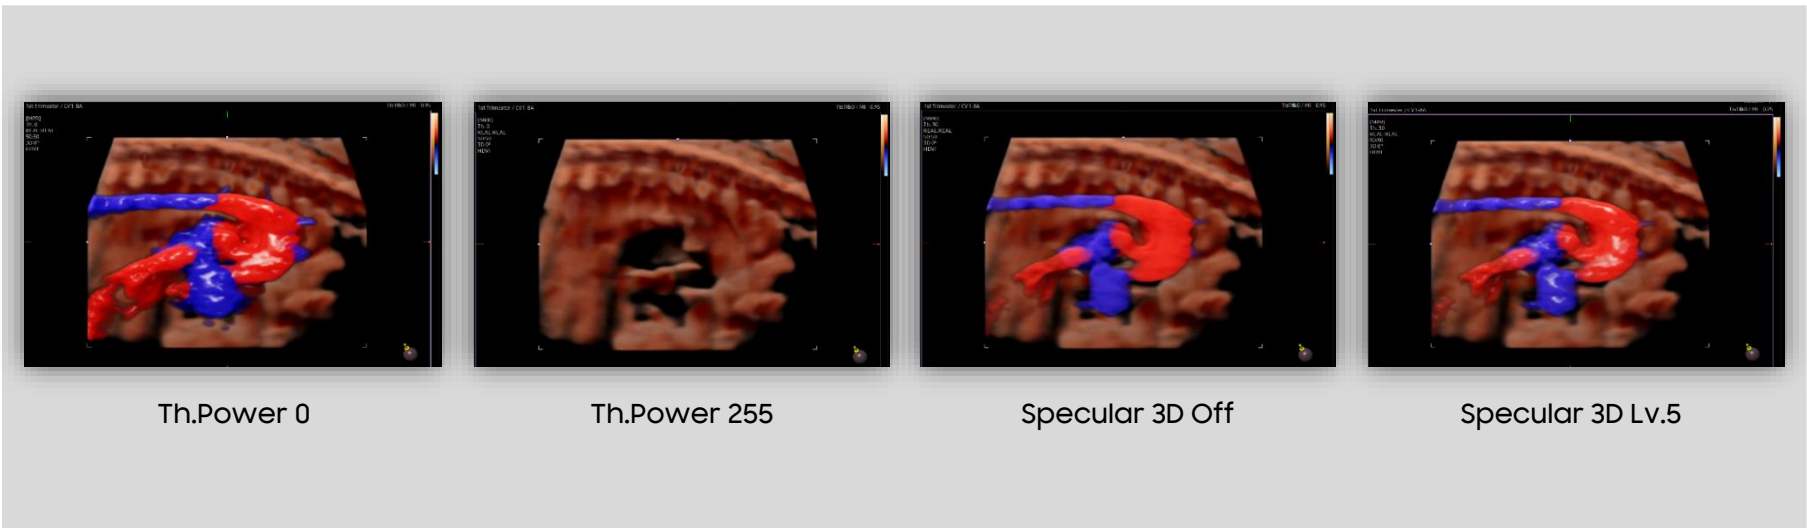


4. Edit CrystalVue Flow™ Preset

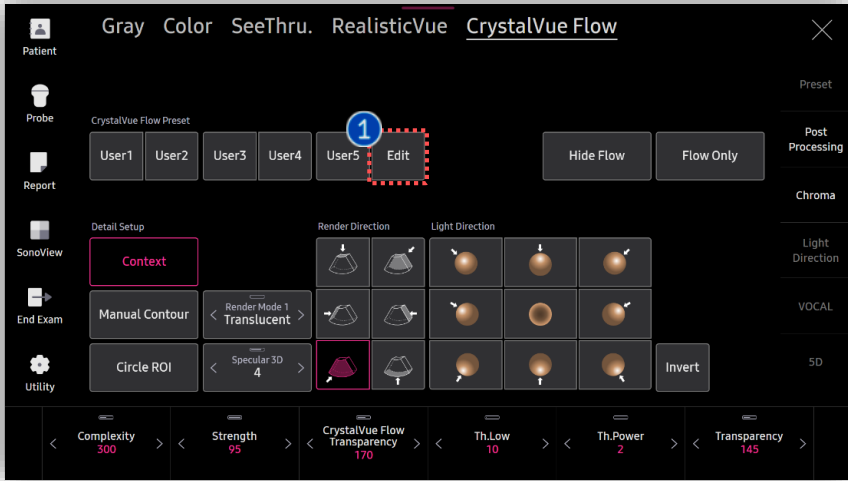

1 Edit

After parameter adjustment, tap [Edit] to save it.

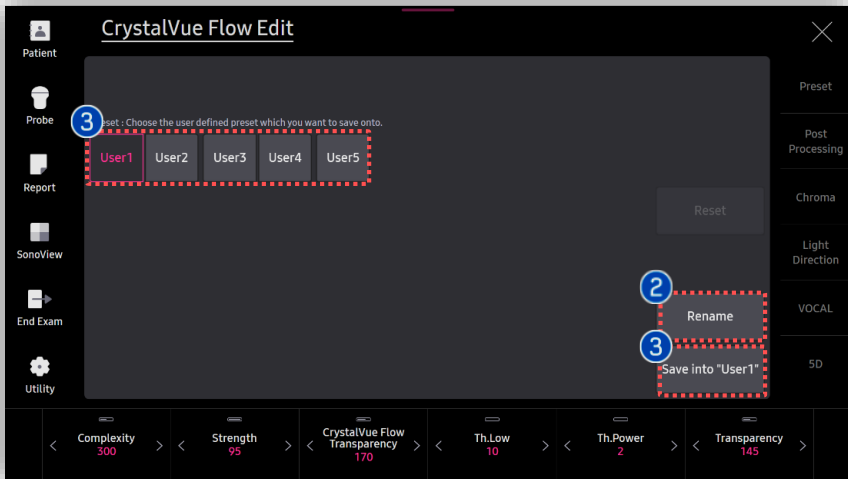

2 Rename

Tap to designate name of the preset.

3 Save into

Tap to save into selected preset.

- The features mentioned in this document may not be commercially available in all countries. Due to regulatory reasons, their future availability cannot be guaranteed.
- Do not distribute this internal document to customers unless relevant regulatory and legal affairs officers approve such distribution.
- This product is a medical device, please read the user manual carefully before use.
- This document is provided to help you understand the feature.
- This User Quick Guide is based on HERA Z20 V1.00.
- Disclaimer: Some Images in this content were obtained from other system.

SAMSUNG MEDISON CO., LTD.

© 2024 Samsung Medison All Rights Reserved.

Samsung Medison reserves the right to modify the design, packaging, specifications, and features shown herein, without prior notice or obligation.